




# SPIKERIGHT™ GUIDE TO CLOSED SYSTEM PUMPS AND PLASTICS

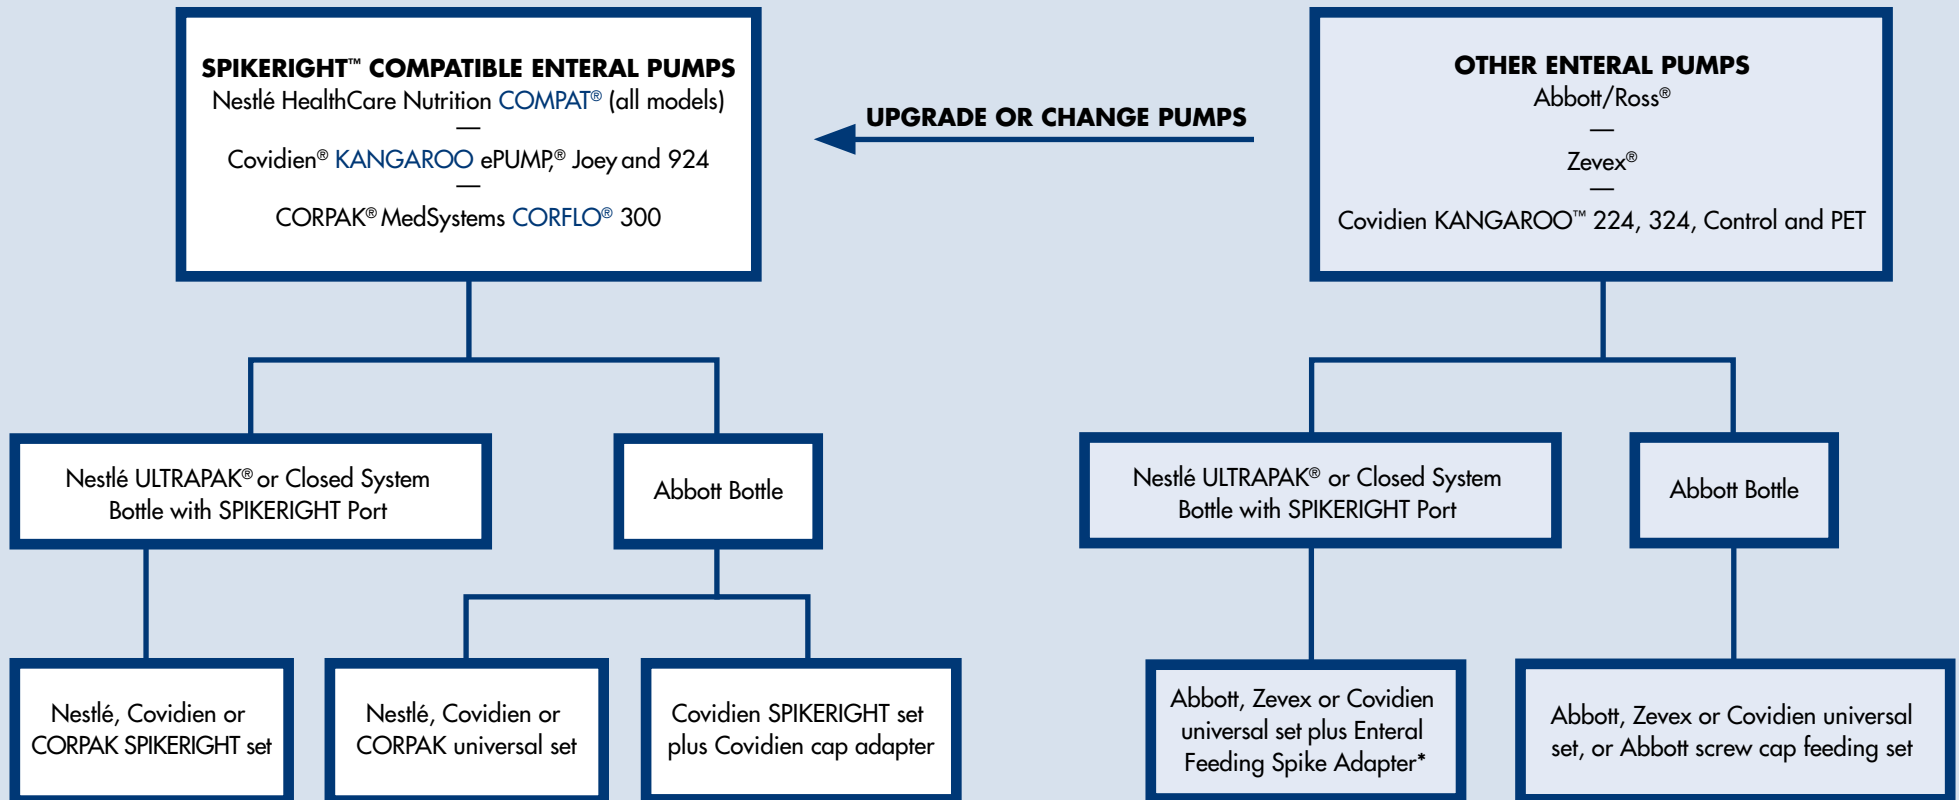

\*The Enteral Feeding Spike Adapter available from Nestlé (22001000) is needed only when administering a Nestlé ULTRAPAK or closed system bottle with SPIKERIGHT port using a noncompatible pump.